

ROMANIAN
NEUROSURGERY

Vol. XXXIV | No. 1 March 2020

Accuracy of 2D fluoroscopy with
preoperative CT fused neuronavigation
in thoracic and lumbar pedicle screw
insertion

Adrian Bălaşa, Corina-Ionela
Hurghiş, Flaviu Tămaş, Ioan-
Alexandru Florian, Levente
Peter, Rareş Chinezu



Accuracy of 2D fluoroscopy with preoperative CT fused neuronavigation in thoracic and lumbar pedicle screw insertion

Adrian Bălașa^{1,2}, Corina-Ionela Hurghiș²,
Flaviu Tămaș², Ioan-Alexandru Florian^{3,4},
Levente Peter², Rareș Chinezu^{1,2}

¹ University of Medicine, Pharmacy, Science and Technology "George Emil Palade", Tirgu Mures, ROMANIA

² Neurosurgery Clinic, Clinical Emergency Hospital, Tirgu Mures, ROMANIA

³ University of Medicine and Pharmacy "Iuliu Hatieganu", Cluj Napoca, ROMANIA

⁴ Neurosurgery Clinic, Clinical Emergency Hospital, Cluj Napoca, ROMANIA

ABSTRACT

Aim: Pedicle screw fixation is an established technique in the lumbar and thoracic area. Fluoroscopy-guided screw placement and subsequently navigation have decreased the rate of misplaced screws, but no technique has wholly eliminated this risk. This paper aims to study the difference between the accuracy of the fluoroscopic guided screw placement to that of the 2D fluoroscopy- preop CT fused neuronavigation guided technique, a lesser-used navigation technique.

Material and Methods: This retrospective study reflects our results using both techniques between March 2018 and March 2019 in both degenerative or traumatic spinal pathology for thoracic and lumbar regions. The accuracy of the screw placement was measured using Mirza grading system on postoperative CT images.

Results: A total number of 56 patients underwent spinal instrumentation surgery. A total of 274 screws were placed with a mean number of 4.89 screws per patient; 199 screws were implanted using neuronavigation and 75 using the freehand-2D fluoroscopy-guided technique. The accuracy rate of pedicle screw placement in the freehand technique guided by 2D fluoroscopy was 88,00%. With the use of neuronavigation, the accuracy increased to 89,96%.

Conclusion: Pedicle screw placement accuracy is higher when guided by CT-fluoro matching neuronavigation compared to freehand fluoroscopy-guided technique and can be used in departments where there is no intraoperative O-arm or 3D fluoroscopy available.

INTRODUCTION

In the past 30 years, spinal surgery has seen a significant increase in the

Keywords

2D fluoroscopy,
CT-fluoro matching,
image guided surgery,
screw accuracy,
transpedicular screw fixation



Corresponding author:
Adrian Bălașa

University of Medicine, Pharmacy,
Science and Technology "George
Emil Palade", Tirgu Mures, Romania

adrian.balasa@umfst.ro

Copyright and usage. This is an Open Access article, distributed under the terms of the Creative Commons Attribution Non-Commercial No Derivatives License (<https://creativecommons.org/licenses/by-nc-nd/4.0/>) which permits non-commercial re-use, distribution, and reproduction in any medium, provided the original work is unaltered and is properly cited.

The written permission of the Romanian Society of Neurosurgery must be obtained for commercial re-use or in order to create a derivative work.

ISSN online 2344-4959
© Romanian Society of
Neurosurgery



First published
March 2020 by
London Academic Publishing
www.lapub.co.uk

development of surgical techniques and instrumentation.

Pedicle screw fixation is an established technique in the lumbar and thoracic area (3). There are many techniques of pedicle screw placement starting from the "free hand technique" described by Kim and Lenke (5,17) to modern techniques that use intraoperative image guidance: 2D fluoroscopy, 2D/3D fluoroscopy navigation, cone beam intraoperative CT navigation or intraoperative MRI navigation (11).

Fluoroscopy-guided screw placement has decreased the rate of misplaced screws from 55% to 21% in the thoracic region and from 40% to 12% in the lumbar region (14). Neuronavigation in spinal surgery further decreased the rate of misplaced screws, but no intraoperative navigation technique

has wholly eliminated this risk (4,7,13).

Neuronavigation using 2D fluoroscopy-CT fusion is a technique used for pedicle screw placement that was described by Sakai (12). This technique uses a preoperative CT thin cut slice scan that is linked via neuronavigation to a set of intraoperative fluoroscopic images and allows for navigation even in the absence of 3D fluoroscopic C-arms or intraoperative CT machines (12). Despite being introduced more than ten years ago, this technique has not seen wide adoption, and no relevant studies are available to assess its efficacy.

This paper aims to study the difference between the accuracy of the fluoroscopic guided screw placement to that of the 2D fluoroscopy-CT fused neuronavigation guided technique.

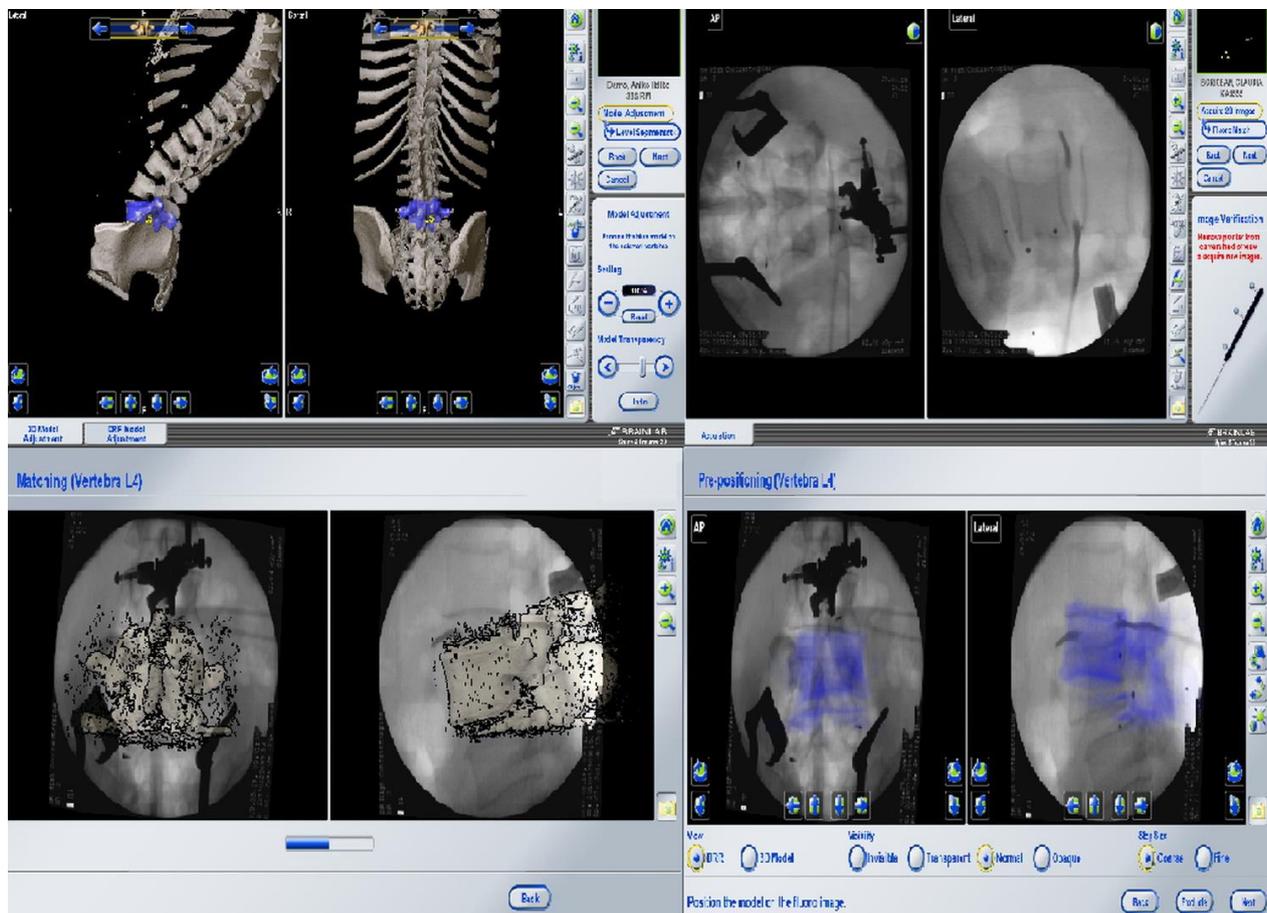


Figure 1: Fusion between the intraoperative fluoroscopy and a 3D model of a vertebra (based on the CT scan) and subsequently registration of the defined vertebra.

MATERIALS AND METHODS

This retrospective study was performed between

March 2018 and March 2019 at the Department of Neurosurgery of the Tîrgu Mureş Clinical Emergency

Hospital, Romania. Patients were operated by a team of multiple neurosurgeons, all with proper levels of spinal instrumentation expertise. The study has included traumatic and degenerative cases in the thoracic and lumbar spine; redo surgeries or repositioning of misplaced screws were not included.

All patients were operated in a prone position using a Bertchtold translucent table (Stryker, Michigan, USA). Intraoperative fluoroscopy was performed in all cases with a Siemens Siremobil Compact L 200 machine (Siemens, Munich, Germany). For cases in which the neuronavigation guided technique was used, a preoperative CT thin cut slice (under 3 mm slices) scan of the operated area was obtained before surgery. A Curve BrainLab (BrainLab, Munich, Germany) neuronavigation system was used in conjunction with a Spine and Trauma software (BrainLab, Munich, Germany) (Figure 1). A fusion between the intraoperative fluoroscopy and a 3D model of a vertebra (based on the CT scan) and subsequently registration of the defined vertebra was performed using Sakai's (12) previously described technique (Figure 1).

Medtronic polyaxially titanium screws (Medtronic, Minnesota, USA) or Stryker (Stryker, Michigan, USA) monoaxial and polyaxially titanium screws with diameters ranging from 4 to 6 mm, and lengths between 40 and 60 mm were used, depending on the spinal level and pedicle width.

There are two commonly used grading systems used for measuring screw placement accuracy: Zdichavsky (18), (9) and Mirza (10) which use postoperative CT images to analyze the pedicle screw placement accuracy. We have chosen to use in our study the Mirza scoring system (Table 2).

Table 1. Demographic distribution.

No. Patients	56	
Sex		
Male	36 (64, 28%)	
Female	20 (35, 72%)	
Age (years)		
Mean	52,76	
Range	20-75 years	
Pathology/Level	Traumatic	Degenerative conditions
Thoracic	15 patients (26,78%)	0 patients (0%)
Thoraco-Lumbar	1 patients (1,78%)	0 patients (0%)

Lumbar	18 patients (32,14%)	17 patients (30,35%)
Lumbo-Sacral	0 patients (0%)	5 patients (8,92%)
Number of screws implanted	CT-fluoro-matching neuronavigation	2D fluoroscopy Freehand
THORACAL	46 (23.11%)	32 (42.66%)
LUMBAR	153 (76.88%)	43 (57.33%)

Table 2. Mirza et al. 2 mm increment grading system.

Classification	Borders
Grade 0 (optimal)	the screw correctly fits the pedicle
Grade 1 (minor)	under 2 mm of displacement
Grade 2 (moderate)	between 2 to 4 mm of displacement
Grade 3 (severe)	over 4 mm of displacement

Postoperative imaging was analyzed by the senior author (AB) and an independent radiologist. Statistical analyses included descriptive (frequency, mean, standard deviation) and inferential statistics. The Shapiro-Wilk test was applied to determine the distribution of the analyzed data series. For analyzing the quantitative variables the t-Student test was applied for unpaired data and for analyzing the qualitative variables the Fisher test was applied. The significance threshold chosen for the p value was 0.05. Statistical analysis was performed using the GraphPad Prism trial variant.

RESULTS

Between March 2018 and March 2019, a total number of 69 patients underwent spinal instrumentation surgery in the thoracolumbar regions for degenerative or traumatic pathology. Out of these, 56 patients (81.16%) had complete documentation and were included in our study. Second surgery for repositioning of screws was necessary in 2 screws (2 cases).

A total of 274 screws were placed with a mean number of 4.89 screws per patient, ranging from 4 screws to a maximum of 10 screws. In our study, traumatic pathology was represented by 60.71% (n=34) of cases, and the lumbar spine was the most frequent region involved with 39.29% of cases (n=35). Table 1 summarizes the clinical data and demographic distribution of the patients.

The CT fluoro matching neuronavigation method was used in 72.63% of cases, which resulted in a total

of 199 screws implanted; the rest of 75 (27.37%) screws were implanted using the "freehand" technique under fluoroscopy guidance. The distribution of screws by region and the type of technique used is seen in Table 1.

The results of the Mirza 2 mm increment staging system are presented in Table 3 for medial and lateral displacement and Table 4 for the correlation between the severity of displacement and anatomic region.

From 20 mispositioned screws implanted under

neuronavigation guidance, 11 screws were in the lumbar area and 9 screws in the thoracic area. The misplaced screws in the thoracic area represented 19.57% of the total number of 46 screws implanted, whilst in the lumbar area, the misplaced screws represented 7.19% of the total of 153 screws implanted. All severely placed screws were in the thoracic area (Table 4). There is a statistically significant association between the region of screw implantation and the malposition rate ($p = 0.023$, Fischer's test).

Table 3. Grade of screw misplacement using the 2 mm increment (Mirza score) classification and screws direction tendency of cortex perforation.

Severity	Minor (%)	Moderate (%)	Severe (%)	Total (%)	P
Lateral misplacement with Neuronavigation	6 (3.01%)	4 (2.01%)	1 (0.50%)	11 (5.52%)	0.55
Lateral misplacement with Fluoroscopy	1 (1.33%)	1 (1.33%)	1 (1.33%)	3 (4%)	
Medial misplacement with Neuronavigation	8 (4.02%)	1 (0.50%)	0 (0%)	9 (4.52%)	0.99
Medial misplacement with Fluoroscopy	5 (6.66%)	1 (1.33%)	0 (0%)	6 (8%)	

Table 4. Grade of screw misplacement using the 2mm increment (Mirza score) classification relative to the vertebral region.

2D Fluoroscopy Freehand	Number of screws (%)	Misplacement rate (%)			p value
		Minor	Moderate	Severe	
Thoracal	32 (42.66)	4 (8.69%)	4 (8.69%)	1 (2.17%)	0.1585
Lumbar	43 (57.33)	10 (6.53%)	1 (0.65%)	0 (0.00%)	
Total	75	20			
CT- fluoro- Matching Neurnavigation					
Thoracal	46 (23.11%)	4 (12.50%)	1 (3.12%)	1 (3.12%)	0.0231
Lumbar	153 (76.88%)	2 (4.65%)	1 (2.32%)	0 (0.00%)	
Total	199	9			

DISCUSSIONS

This study tries to reflect our experience in transpedicular screw implantation. We focused on the accuracy of transpedicular screw implantation using the two implantation procedures that are used at our institution: freehand technique under fluoroscopy guidance and neuronavigation with CT-2D fluoro-matching.

There are few articles in the literature about pedicle screw implantation that include CT-fluoro-matching neuronavigation or compare this technique with the freehand technique under fluoroscopic guidance (15), and to our knowledge this is the first series presented. This might be

because intraoperative 3D fluoroscopy or intraoperative CT has become widely available.

Scoring the screw misplacement is still a difficult task as there are reported more than 35 classifications that analyze pedicle screw misplacement and, in most of them, there is no clear description of the assessment methods used to determine the accuracy of the pedicle screw positioning (2,6). Evermore there are publications showing that moderate lateral or medial displacement of the screws with violation of the pedicle cortex does not commonly relate with neurologic, vascular, and/or visceral complications (8).

We have chosen Mirza scoring system(10) because this seems to be the most widely accepted and one of the most precise scale for scoring pedicle screw placement. (1)

Our overall accuracy rate of pedicle screw placement using the freehand technique guided by 2D fluoroscopy was 88.00%. With the use of the neuronavigation, the accuracy increased to 89.96%. Nevertheless, our results are comparable to different other papers:

- The screw misplacement rate in our study was of about 12% in the fluoroscopy technique group, and pedicle cortex perforation over 4 mm (severely misplaced screw) was seen in 1.33%, comparable to the results previously published by Guedes and Verma (2),(16).
- In our CT-fluoro navigation group, a slight increase in the overall accuracy was noted. Even if this increase in accuracy is not statistically significant, these results are similar to the ones of Kosmopoulous (6), showing over 90% accuracy rate for both techniques, and might be partially explained by good fluoro screw positioning technique.
- Gelalis (3) concluded that neuronavigation increases the accuracy of pedicle screw placement and when using freehand technique there is an increased tendency of medial perforation of pedicle cortex as opposed to neuronavigation where the tendency is to perforate the cortex laterally which decreases the risk of neurological complication even in case of inaccuracy. Our results seem to reconfirm this as in the CT-fluoro group we noted a slight increase in the lateral displacement (5,52% vs. 4%) but also a 50% reduction of medial misplacement (4.52% vs. 8%) (Table 3.)

There are also inherent limitations to CT-fluoro matching neuronavigation technique: due to the acquisition of the preoperative spine CT in the supine position and the prone position in the operating room, a spine displacement most likely occurs and interferes with the accuracy(8). Scanning patients in prone position or spine curvature detection algorithms might further improve this technique. Inaccuracies are also given by the need to fuse a 3D vertebral body model to a 2D intraoperative fluoroscopy, and a less than perfect thoracic imaging allows for navigation errors and screw misplacement

that is higher than the rate we obtained in lumbar spine, but still lower than freehand fluoroscopy technique.

CONCLUSION

Despite its shortcomings, the CT-fluoro matching technique has similar or slightly better results than freehand fluoroscopy and can be used in departments where there is no intraoperative O-arm or 3D fluoroscopy available and a more affordable neuronavigation solution is required.

CONFLICTS OF INTEREST

The authors of this paper state that they have no conflict of interests to disclosure.

ABBREVIATIONS

MRI: magnetic resonance imaging
 CT: computer tomography
 2D: two-dimensional
 3D: three-dimensional

REFERENCES

1. Aoude AA, Fortin M, Figueiredo R, Jarzem P, Ouellet J, Weber MH: Methods to determine pedicle screw placement accuracy in spine surgery: a systematic review. *Eur. Spine J.* 24: 990–1004, 2015.
2. De Paula Guedes V, Manffra EF, Aguiar LR: Image-guided surgery in the spine: Neuronavigation vs. fluoroscopy. *Coluna/ Columna* 14: 181–185, 2015.
3. Gelalis ID, Paschos NK, Pakos EE, Politis AN, Arnaoutoglou CM, Karageorgos AC, Ploumis A, Xenakis TA: Accuracy of pedicle screw placement: A systematic review of prospective in vivo studies comparing free hand, fluoroscopy guidance and navigation techniques. *Eur. Spine J.* 21: 247–255, 2012.
4. Karhade A, Vasudeva, Pompeu, Lu: Image Guided Spine Surgery: Available Technology and Future Potential. *Austin Neurosurg Open Access* 3: 1043–1, 2016.
5. Kim YJ, Lenke LG, Bridwell KH, Cho YS, Riew KD: Free Hand Pedicle Screw Placement in the Thoracic Spine: Is it Safe. *Spine (Phila. Pa. 1976)*. 29: 333–342, 2004.
6. Kosmopoulos V, Schizas C: Pedicle Screw Placement Accuracy. *Spine (Phila. Pa. 1976)*. 32: E111–E120, 2007.
7. Laine T, Mäkitalo K, Schlenzka D, Tallroth K, Poussa M, Alho A: Accuracy of pedicle screw insertion: A prospective CT study in 30 low back patients. *Eur. Spine J.* 6: 402–405, 1997.
8. Liu H, Chen W, Liu T, Meng B, Yang H: Accuracy of pedicle screw placement based on preoperative computed tomography versus intraoperative data set acquisition for spinal navigation system. *J. Orthop. Surg.* 25: 1–8, 2017.
9. Marios Theologou1 2, , Theologos Theologou1 , Dimitrios

- Zevgaridis¹, Nikolaos Skoulios², Slavisa Matejic³ CT: Pedicle screw placement accuracy impact and comparison between grading systems *Marios. Surg. Neurol. Int.* 8: 1–7, 2017.
10. Mirza SK, Wiggins GC, Kuntz IV C, York JE, Bellabarba C, Kwon MA, Chapman JR, Shaffrey CI: Accuracy of thoracic vertebral body screw placement using standard fluoroscopy, fluoroscopic image guidance, and computed tomographic image guidance: A cadaver study. *Spine (Phila. Pa. 1976)*. 28: 402–413, 2003.
 11. Moses ZB, Mayer RR, Strickland BA, Kretzer RM, Wolinsky J-P, Gokaslan ZL, Baaj AA: Neuronavigation in minimally invasive spine surgery. *Neurosurg. Focus* 35: E12, 2013.
 12. Sakai Y, Matsuyama Y, Yoshihara H, Nakamura H, Nakashima S, Ishiguro N: Simultaneous registration with ct-fluoro matching for spinal navigation surgery. A case report. *Nagoya J Med Sci* 68: 45–52, 2006.
 13. Shin MH, Hur JW, Ryu KS, Park CK: Prospective Comparison Study between the Fluoroscopy-guided and Navigation Coupled with O-arm - Guided Pedicle Screw Placement in the Thoracic and Lumbosacral Spines. *J. Spinal Disord. Tech.* 28: E347–E351, 2015.
 14. Tehli O, Harman F, Temiz C, Kacar Y, Kazanci B, Daneyemez M, Solmaz I, Kural C: The Use of Neuronavigation and Intraoperative Imaging in Spinal Stabilization Surgery. *Turk. Neurosurg.* 26: 771–776, 2016.
 15. Tjardes T, Shafizadeh S, Rixen D, Paffrath T, Bouillon B, Steinhausen ES, Baethis H: Image-guided spine surgery: state of the art and future directions. *Eur. Spine J.* 19: 25, 2010.
 16. Verma SK, Singh PK, Agrawal D, Sinha S, Gupta D, Satyarthee GD, Sharma BS: O-arm with navigation versus C-arm: a review of screw placement over 3 years at a major trauma center. *Br. J. Neurosurg.* 30: 658–661, 2016.
 17. Wagner SC, Morrissey PB, Kaye ID, Sebastian A, Butler JS, Kepler CK: Intraoperative pedicle screw navigation does not significantly affect complication rates after spine surgery. *J. Clin. Neurosci.* 47: 198–201, 2018.
 18. Zdichavsky M, Blauth M, Knop C, Graessner M, Herrmann H, Krettek C, Bastian L: Accuracy of pedicle screw placement in thoracic spine fractures - Part I: Inter- and intraobserver reliability of the scoring system. *Eur. J. Trauma* 30: 234–240, 2004.